




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁶ : A61B 17/064	A1	(11) International Publication Number: WO 99/01071 (43) International Publication Date: 14 January 1999 (14.01.99)
(21) International Application Number: PCT/EP98/04183 (22) International Filing Date: 2 July 1998 (02.07.98) (30) Priority Data: 08/887,130 2 July 1997 (02.07.97) US (71) Applicant: BIONX IMPLANTS OY [FI/FI]; Runeberginkatu 3 A1, FIN-33710 Tampere (FI). (72) Inventors: TORMALA, Pertti; Nestori Sarrin Katu 1, FIN-33720 Tampere (FI). POHJONEN, Timo; Nosturi-naraitti 2 B 17, FIN-33720 Tampere (FI). TAMMINMAKI, Markku; Kukkolankatu 23 B 12, FIN-33400 Tampere (FI). (74) Agent: BOULT WADE TENNANT; 27 Fumival Street, London EC4A 1PQ (GB).		(81) Designated States: AU, CA, JP, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE). Published <i>With international search report.</i>

(54) Title: SURGICAL FASTENER FOR TISSUE TREATMENT

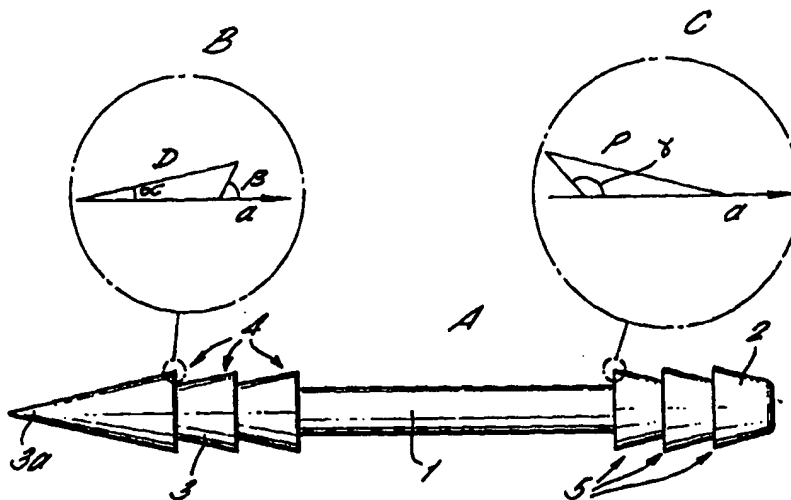

(57) Abstract

The disclosure relates to a surgical fastener or device (implant) formed in the shape of an arrow comprising a shaft (1) with a proximal (first) portion (2) having protrusions (5) and a blunt end and a distal (second) portion (3) having protrusions (4) and a pointed end (3a), the protrusions of the proximal and distal portions configured to lock the implant in a position inside a soft and/or tough tissue according to the use of the implant. The implant may be manufactured of a polymer or a polymeric compound which is substantially (bio)absorbable in tissue conditions and contains oriented reinforcing structure or the like of a polymer or polymeric compound or ceramic bioglass compound. The surgical implant of the invention is particularly but not solely intended to be used in repair surgery of traumas of soft and/or tough tissues containing fibrous structures, such as knee meniscal tissues.

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakhstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

SURGICAL FASTENER FOR TISSUE TREATMENT

FIELD OF THE INVENTION

The present invention relates to a surgical fastener or device (implant) formed in the shape of an arrow comprising a shaft with a proximal (first) portion having protrusions and a blunt end and a distal (second) portion having protrusions and a pointed end, the protrusions of the proximal and distal portions configured to lock the implant in a position inside a soft and/or tough tissue according to the use of the implant. The implant may be manufactured of a polymer or a polymeric compound which is substantially (bio)absorbable in tissue conditions and contains oriented reinforcing structure or the like of a polymer or polymeric compound or ceramic bioglass compound.

The surgical implant of the invention is particularly but not solely intended to be used in repair surgery of traumas of soft and/or tough tissues containing fibrous structures, such as knee meniscal tissues.

BACKGROUND ART

With reference to the prior art in the field it has been shown that fixation of meniscus traumas like ruptures and lesions by suturing with absorbable sutures gives better results than removal of traumatized meniscal tissue, see e.g. N.A. Palmeri, T.F. Winters, A. E. Joiner and T. Evans, "The Development and Testing of the Arthroscopic Meniscal Staple", Arthroscopy, Vol. 5, No. 2, 1989, p. 156 (Ref. 1). However, arthroscopic suturing is a complicated and tedious technique where risks

for the patient are significant because of danger to vessels and nerves. Additionally, the suturing of meniscus ruptures leaves a single or several loops of sutures, which can irritate joint cavity tissues. Therefore, for a long time surgeons have desired an absorbable meniscus lesion fixation device, like a staple or fastener, which has the advantages of absorbable suturing techniques but which can be used more rapidly and safely than sutures.

Several research groups have tried to develop absorbable meniscus lesion fixation devices such as clamps. However, the various demands upon such a device are high. It must be strong enough to maintain good contact of lesion tissues after the operation so that rapid healing occurs. The device must retain its strength long enough for good healing. It must be absorbed without causing complications that would prevent the healing of the lesion. Additionally, the installation of the device should be easy and rapid and should cause minimum operational trauma. Because of these high demands, an optimal absorbable meniscus lesion fixation device has not been developed yet. Palmeri et al. reported in Ref. 1 the development of a method of meniscal repair using arthroscopically applied absorbable fasteners. However, the reported method was complicated because the final design used cannulation of the staple for needle-guided placement. Additionally, staple fracture, migration and articular abrasion was found.

With regard to implants known in this field, reference is made to U.S. Pat. No 4,873,976 which discloses an arrow-like implant particularly intended for the surgical repair of meniscal ruptures. However, the arrow-like implant according to this publication has the disadvantage that particularly its proximal end (stem) is shaped as a plate in a way that the direction of the main plane of the plate is perpendicular to the longitudinal direction of the arrow's body. Because of this fact, it is particularly difficult to install the implant, because the channel used to install the implant must have the cross-sectional shape of the stem; it is difficult to guide the implant in the installation channel, because the guiding effect is substantially brought upon the stem only, and not the body of the arrow. Furthermore, the structure of the stem causes tissue irritation and abrasion, particularly when placed in connection with the

meniscus because the stem is usually left protruding to a high degree from the outer surface of the meniscus.

5 Bays et al. (U.S. Pat. Nos. 4,884,572 and 4,895,141) describe a surgical-repair tack and applicator and method of using them. The tack has a barb member, a shaft portion and a grip portion. The tack is made of biodegradable material having a degradation time selected to coincide with the healing time of the tissue. In an alternate embodiment, the tack's barb comprises a continuous helical barb. A disadvantage of this tack is that the grip portion is bulky and may remain on
10 meniscal surface causing irritation inside a joint cavity.

The method and apparatus for repairing a meniscal tear disclosed by Winters (U. S. Pat. No. 5,059,206) comprises a fastener having protrusions or barbs that is applied to a meniscal tear with a delivery device. The delivery device has a flexible tip
15 that is manipulable through a curved radius to enable the surgeon to insert the device into the central part of the knee and then extend the fastener radially outward into and across a meniscal tear. Also in this case the proximal end of the fastener is bulky and protrudes partially above and/or below the outer surface of the meniscus.

20 Tamminmaki et al. (U.S Pat. No. 5,562,704) disclose an arrow-like bioabsorbable implant particularly intended for the surgical repair of meniscal ruptures. This implant does not have the guiding or abrasion problems that implants of U.S. Pat. No. 4,873,976 or U.S. Pat. No. 5,059,206 may have. However, a disadvantage of U.S. Pat. No. 5,562,704 is that the proximal part of the implant (the wings) preferably remains on the surface of the meniscus, so that when the wings
25 break as a consequence of bioabsorption, the broken wings may irritate knee joint tissues. If the proximal part with the wings is desired to be located inside of meniscal tissue, the surface capsule of the meniscus must be cut horizontally with a special cutting blade. This lengthens the operation time and causes substantial damage to the
30 meniscus surface.

U.S. Pat. No. 5,569,252 describes a fastener, an installation device, and

method for repairing tears in the soft tissue of a patient, including meniscal tears. The fastener has a variable-pitch helical protrusion along a central portion that decreases from the distal end to the proximal end, which can serve to bring two sides of the tear into apposition as the fastener is advanced across the two sides of the tear in a screwing motion. This implant, which needs a screwing motion for installation, is slow and tedious to use arthroscopically and the turning of the implant through fibrous tissue, such as meniscus tissue, has the risk that the fibrous tissue may twist around the turning implant, hindering or preventing the installation of the implant.

Orthopedic and Musculoskeletal Markets Biotechnology and Tissue Engineering, Medical Data International, Inc., Irvine, California, USA, Feb 1997, p.1-17 describes a bioabsorbable device for meniscal repair. This device has two legs with molded barbs that are attached by a flexible member composed of a resorbable suture. The device is installed into a meniscus with an arthroscopical tool so that the legs penetrate the rupture of meniscus to hold the edges together. The disadvantage of this device is that the suture loop remains on the surface of meniscus where it can cause irritation. Additionally, the two-leg device requires a bulky installation tool which makes arthroscopical installation of the device difficult.

SUMMARY OF THE INVENTION

It is an object of the present invention to provide a bioabsorbable fastener that allows a minimally invasive method for repairing a tear in soft or tough tissue.

It is a further object to provide such a fastener that is rapid and easy to install and gives a strong and safe fixation of the tissue tear and that may be made from a nontoxic, biocompatible bioabsorbable polymer, polymer alloy or fiber reinforced polymer composite, specially designed to maintain its structural integrity during the healing of the tear and to prevent tissue abrasion.

It is an additional object to provide such a fastener having a shape designed to compress the tear

It is a further object to provide a device (fastener) which will be shot totally inside of soft or tough tissue, like meniscal tissue, to penetrate the tissue (meniscal) tear and to hold the ruptured edges together

5 These and other objects are attained with the fastener of the present invention.

The fastener of the present invention is designed for repairing a tear in soft and/or tough tissue of a patient, such as a tear of the meniscus within the knee.

10

The implant has a shaft with a proximal (first) portion formed with protrusions in relation to the surface of the shaft and having a blunt end and a distal (second) portion formed with protrusions in relation to the surface of the shaft and having a pointed end. The purpose of the protrusions is to arrest (lock) the implant inside of the soft and/or tough tissue after installation.

15

Accordingly protrusions emerge from both the proximal and distal portions of the device. The protrusions are typically barbs, scales, threads, serrations, ridges or the like. The protrusions at the distal portion of the shaft of the device prevent the installed device from slipping out of the meniscal tissue in the direction opposite to the direction of installation and the protrusions at the proximal portion of the shaft prevent the installed device from further penetrating the meniscal tissue in the direction of installation. This behavior is achieved with the special geometry of the protrusions.

20

25

In a preferred embodiment the protrusions of the distal portion of the shaft of the device are formed so that they facilitate the slipping of the device into the meniscus during insertion but they resist the slipping of the device in the direction opposite to the installation direction. On the other hand, the protrusions of the proximal portion of the shaft of the device are formed so that they stop the device inside of meniscal tissue when the device has been shot into the meniscus with the delivery (installation) tool. Both sets of protrusions, acting together, exert an

30

advantageous compression to the ruptured surface when the device is shot into the meniscus and across the rupture. This compression serves to close the rupture and promotes healing.

5 A further advantageous feature of the device is that the surface of the shaft may include longitudinal ridges.

Protrusions that are manufactured on these ridges are more effective at preventing unwanted movement of the installed fastener and maintaining compression
10 of the rupture. Because of their increased prominence, it is also easier to manufacture protrusions on ridges. Moreover, the ridges unexpectedly promote healing of the rupture by providing channels along the interiors of the ridges through which beneficial blood flow can occur along the length of the device. These channels, which are about .05-.5 mm wide, act as capillaries, transporting blood from
15 the highly vascularized distal portion of the meniscus to the poorly vascularized proximal portion of the meniscus. Further, the ridges help to guide the fastener through the cannula of the installation instrument and into the meniscal or other soft tissue during installation.

20 **BRIEF DESCRIPTION OF THE DRAWINGS**

FIGS. 1-6 illustrate fasteners (devices) in accordance with the invention. FIGS. 7-10 describe different ridge profiles in fasteners in accordance with the invention. FIGS. 11A-D illustrate as a cross-section the installation of the fastener of
25 the invention into the torn meniscus. FIGS 12-13 illustrate the fibrous structure of the meniscus. FIGS 14-15 illustrate the orientation of the fibrous structure of the meniscus in relation to an installed fastener of the invention.

30 **DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS**

A description of the preferred embodiments of the present invention is presented with reference to FIGS. 1-15.

The preferred exemplary embodiment of the present invention comprises a fastener and method for repairing a soft or tough, tissue, like a knee meniscal tear in a human patient.

5 FIG. 1 illustrates, as viewed from the side, a preferred embodiment of the fastener. It is designed to have an arrow shape, and it comprises a shaft 1, whose proximal portion 2 is formed with a blunt end for the purpose of providing the impact surface required for the instrument used in the installation of the implant and whose distal portion 3 is formed with a head with a sharp tip 3a. The distal portion
10 comprises distal protrusions 4 with respect to the shaft 1. The distal protrusions are here sharp-profile threads which go around the shaft. The purpose of the proximal portion 2 is to stop the implant inside of the meniscus, typically just below the surface of the meniscus during the final stage of the installation. To fulfill this task, the proximal portion 2 is equipped with proximal protrusions 5, which stop the device
15 and prevent its further sinking into the meniscus, when the pushing effect of the delivery tool stops. FIG. 1B illustrates the cross-section of a distal protrusion showing that the angle α between a tangent to the distal surface of the protrusion (D) and the longitudinal axis (a) of the fastener in the proximal direction is relatively small, less than 45° and preferably less than 30° to facilitate the easy penetration of
20 the tip of the fastener into the meniscal tissue. On the other hand, the angle β between a tangent to the proximal surface of the protrusion (D) and the axis (a) in the proximal direction is $<90^\circ$ to guarantee the effective prevention of slipping of the fastener back in the direction opposite to the installation direction after installation of the fastener. On the other hand, according to FIG. 1 C, in the case of the proximal
25 protrusion, P, the value of angle γ is big ($>90^\circ$) to create a strong locking force, which stops the fastener inside of the meniscal tissue after the installation procedure.

 Accordingly, the proximal and distal protrusions 5 and 4 effectively lock the device inside of the meniscus preventing its movement both in the direction of
30 installation and in the direction opposite to it. Additionally, the installation compresses the rupture surface (see FIGS. 11A-D) because the proximal protrusions 5 push the proximal side of the rupture against the distal side of the rupture during

the final phase of installation.

Because the whole device is located inside of the meniscus and the proximal end of the device is relatively small, the risks of prior art devices regarding the complications originating from the presence of the bulky proximal part of the device on the meniscal surface, are eliminated.

FIG. 2 illustrates another preferred embodiment of the fastener. Here the proximal protrusions (6) and the distal protrusions (7) comprise a plurality of small barbs emerging from the surface of the proximal and distal portions of the shaft. The fasteners of FIGS. 1 and 2 can be pushed into meniscal tissue through a cannula with a circular cross-section, which makes the manufacturing of the cannula relatively easy.

FIG. 3A illustrates, as viewed longitudinally from the side and FIG. 3B illustrates, as viewed from above, a fastener which has proximal and distal, ridge-like protrusions (8,9) and whose middle part 10 has been flattened, so that the fastener has a cross-like profile when viewed from the direction of the distal tip of the fastener, according to FIG. 3C. This type of fastener allows for excellent guidance inside of an installation cannula whose inner cross-section corresponds to the cross section of the fastener according to FIG. 3C.

The surface of the fastener can also include longitudinal ridges, into which the arresting means can be machined or molded. FIG. 4A shows a side-view perspective of such a fastener having on its surface four longitudinal ridges (R), which are arranged onto the surface of the fastener according to FIG. 4B which gives the cross-section of the fastener in the plane A-A of FIG. 4A.

The proximal and distal protrusions (like barbs) can be machined effectively into the longitudinal ridges.

It is evident that other types of proximal and distal protrusions, than those

described in FIGS. 1-4, can be used in the fasteners of the invention. E.g., both of the slopes of protrusions can be curved, as is illustrated in FIG 5. The protrusions can also be both stiff and sharp-pointed as is illustrated in FIG 6.

5 There are numerous possible arrangements for the longitudinal ridges on the surface of the fastener. Also the geometry of the ridges can be varied to influence the gripping capacity of barbs or other protrusions inside of meniscal or other soft tissue. FIGS. 7-10 illustrate some preferred embodiments of the cross-sectional structures of ridged fasteners.

10

FIG. 11A-D illustrate a preferred method for installing fasteners of the invention into ruptured meniscal tissue. Figure 11A illustrates, as viewed from the side, a meniscus with a rupture, 12, separating the meniscus into a proximal side, 11', and a distal side, 11". As seen in FIG. 11B during the operation the tip, 13" of a cannula 13 is pushed into the knee joint through a small incision and the tip is located on the surface of the proximal part of the meniscus 11' (in relation to the rupture 12).

15

As seen in FIG. 11C, piston 15 moves to the left (distally) and pushes the fastener 14 through the hole 13' inside of cannula 13. The piston 15 can be accelerated to a high speed so that the piston 15 pushes (shoots) the fastener 14 with a high speed into the meniscus as is illustrated in FIG. 11D. The piston 15 stops at the final stage of its movement (by way of, e.g., a stopper [not shown] at the proximal end of the piston 15), typically so that the tip of the piston protrudes out of the tip 13" of cannula 13 ca. 0.5-1 mm, to push the fastener totally inside of the meniscal tissue. When the location of the cannula tip 13" on the meniscal surface is selected in a proper way, typically 2-4 mm in front of the meniscal tear 12, and the direction of the cannula is proper, the fastener penetrates the proximal meniscus part 11', the tear plane 12 and closes the tear with the compression force created with the installation push. According to FIG. 11D the piston 15 pushes and forces the fastener 14 totally inside of the meniscal tissue. When the proximal portion 16 of the fastener is forced inside of the meniscal tissue, the proximal protrusions 16' create the pushing force into the proximal part of meniscus 11', closing the rupture 12. As soon

25

20

30

as the piston 15 stops (typically 0.5-1 mm below the surface of the meniscus) the proximal protrusions 16' stop the fastener and prevent its further movement into meniscal tissue. On the other hand, the distal portion of the device 17 is pushed across the rupture 12 and into the distal side of the meniscus 11", where the distal protrusions 17' prevent the slipping of the fastener back in the direction opposite to the installation direction. Accordingly, the rupture 12 is closed effectively, the fastener is locked to its position to keep the rupture 12 closed and the whole fastener has been buried inside of meniscal tissue to eliminate the risks related to implant parts located on the surface of the meniscus.

It is typical that the microstructure of a meniscus contains reinforcing collagen fibers. Inside of a meniscus, many collagen fibers are oriented in a horizontal plane nearly parallel to the lower surface of the meniscus. If the horizontal collagen fibers are examined in a cut cross-section of a meniscus (as shown in FIGS. 11-11D) their cut ends can be seen microscopically as points on the cross-sectional surface, according to FIG. 12. The typical vertical meniscus lesion (rupture) 12 develops along the long axes of collagen fibers, because the binding forces between collagen fibers are relatively weak.

If the internal collagen fiber structure of a meniscus is examined from the direction of the long axis of the fastener, i.e., from the direction from which the fastener enters the meniscus, the collagen fibers are seen as parallel, horizontal fiber bundles, as is shown schematically in FIG. 13.

Because of the special arrangement of reinforcing horizontal collagen fibers inside of the meniscus, shown schematically in FIGS. 12 and 13, it is important that the protrusions are located at least on the upper and lower surfaces of the proximal and distal portions of the fastener, so that as the fastener penetrates into the meniscal tissue, the protrusions grab the horizontal collagen fiber bundles, locking the fastener in place. This is shown schematically in FIG. 14 as a meniscal cross-section. In FIG. 15 the fastener - horizontal collagen fiber relationship is viewed from the direction from which the fastener enters the meniscus, showing how the protrusions 18,

protruding from the upper and lower surfaces of the shaft of the fastener 19, lock themselves effectively between horizontal collagen fibers 20

5 Of course, it is well known that the meniscus also includes oriented fibers that are not horizontal. For example, the meniscus can also contain fibers having radial or oblique orientations. The collagen fibers form an essentially three-dimensional network in the meniscus, with the horizontal fibers being of particular importance with regard to using the present invention for treating the typical vertical (bucket handle) tears that occur.

10

The bioabsorbable implants of this invention can be manufactured of bioabsorbable polymers, copolymers or polymer mixtures or alloys with melt molding methods known in the prior art. It is also possible to use the techniques of U.S. Pat. No. 4,743,257 to mold in a compression or injection mold absorbable fibers and
15 binding polymer together to create a fiber-reinforced or especially a self-reinforced structure. The implants of this invention can be molded in a single compression molding cycle, or the protrusions can be machined on the surface of a fastener after the molding cycle.

20

The oriented or self-reinforced structure can also be created during extrusion or injection molding of absorbable polymeric melt through a suitable die or into a suitable mold at high speed and pressure. When cooling occurs at suitable conditions, the flow orientation of the melt remains in the solid material as an oriented or self-reinforcing structure. In an advantageous embodiment, the mold can
25 have the form of the implant, but it is also possible to manufacture the implants of the invention by machining (possibly using heat) injection-molded or extruded semifinished products.

30

It is advantageous to make the implants of melt-molded, solid state drawn or compressed, bioabsorbable polymeric materials, which are described e.g. in United States Patent No. 4,968,317 or 4,898,186.

The reinforcing fibers of the implant can also be ceramic fibers, like bioabsorbable hydroxyapatite or bioglass fibers. Such bioabsorbable, ceramic fiber reinforced materials are described e.g. in European Patent Application No. 0146398 and in WO 96/21628.

5

The oriented or self-reinforced or otherwise fiber reinforced implants of this invention can be manufactured by molding the reinforcement fiber-polymer matrix to the final product in a mold, whose mold cavity has the form of the final product or the final form can be machined mechanically (possibly also using heat) on a preform, such as a melt-molded and solid-state drawn rod, as is described e.g. in United States Patent No. 4,968,317.

10

In some advantageous embodiments of this invention, the orientation and/or reinforcing elements of the self-reinforced structure are mainly oriented in the direction of the long axis of the shaft of the implant. The reinforcement elements may extend into any protrusions or ridges of the implant. The reinforcement elements can also turn spirally around the long axis of the implant. Also other different orientations of reinforcement elements in elongated samples which are familiar from composite technology can be applied to the present invention. However, a general feature of orientation, fiber-reinforcement or self-reinforcement of the implants of this invention is that many of the reinforcing elements are oriented in such a way that they can carry effectively the different external loads (such as tensile, bending and shear loads) that are directed to the healing rupture (for example, loads to a meniscus caused by the movements of the patient's knee).

15

20

25

According to an advantageous embodiment of the invention, the meniscal repair implant, or a special coating layer on its surface, may contain one or more bioactive substances, such as antibiotics, chemotherapeutic substances, angiogenic growth factors, substances accelerating the healing of the wound, growth hormones and the like. such bioactive meniscal repair implants are especially advantageous in surgical use, because they chemically contribute to the healing of the lesion in addition to providing mechanical support.

30

35

5 The oriented and/or reinforced materials of the implants typically have tensile strengths of 100-2000 MPa, bending strengths of 100-600 MPa and shear strengths of 80-400 MPa. Additionally, they are usually stiff and tough. These mechanical properties are superior to those of non-reinforced absorbable polymers which typically show strengths between 40 and 100 MPa and are additionally either very flexible or brittle (see e.g. Ref 3S Vainionpaa, P. Rokkanen and P. Tormala, "Surgical Applications of Biodegradable Polymers in Human Tissues", Progr. Polym. Sci 14 /1989, pp. 679-716).

10 The implants of the present invention may be sterilized by any of the well known sterilization techniques, depending on the type of material used in manufacture of the implant. Suitable sterilization techniques include heat or steam sterilization, radiation sterilization such as cobalt 60 irradiation or electron beams, ethylene oxide sterilization, and the like.

15

After the description above of the present invention and certain specific embodiments thereof, it will be readily apparent to those skilled in the art that many variations and modifications may be made to the present invention without departing from the spirit and scope thereof.

What is Claimed Is:

1. A fastener for body tissue repair comprising: a shaft comprised of a proximal portion, having an upper surface and a lower surface, and a distal portion, said distal portion having a sharpened tip and one or more first protrusions, wherein said first protrusions have proximal surfaces configured to arrest the movement of the shaft in the proximal direction and distal surfaces configured to permit the movement of the shaft in the distal direction, said proximal portion having second protrusions on the upper surface and lower surface of the proximal portion, wherein said second protrusions have distal surfaces configured to arrest the movement of the shaft in the distal direction.

2. A fastener according to claim 1, wherein the angle formed between a tangent to the distal surfaces of the first protrusions and the shaft, in the proximal direction, is less than 45° , the angle formed between a tangent to the proximal surface of the first protrusions and the shaft, in the proximal direction, is less than 90° , and the angle formed between a tangent to the distal surfaces of the second protrusions and the shaft, in the proximal direction, is greater than 90° .

3. A fastener according to claim 1 or claim 2, the shaft further comprising one or more longitudinal ridges along said proximal portion and said distal portion, wherein said first protrusions protrude from said one or more longitudinal ridges, the said second protrusions protrude from said one or more longitudinal ridges.



4. A fastener according to claim 3, wherein the one or more longitudinal ridges are positioned between the distal and proximal portions of the shaft.

5. A fastener according to any of claims 1 to 4, wherein the fastener comprises a bioactive material.

6. A method for the repair of a rupture in a meniscus, using the fastener of claim 1, comprising the steps of:

- 3 aligning a the fastener of claim 1 on the surface of the meniscus;
- 4 and pushing the fastener into the meniscus so that the fastener is
- 5 embedded within the meniscus and bridges the rupture.

1/6

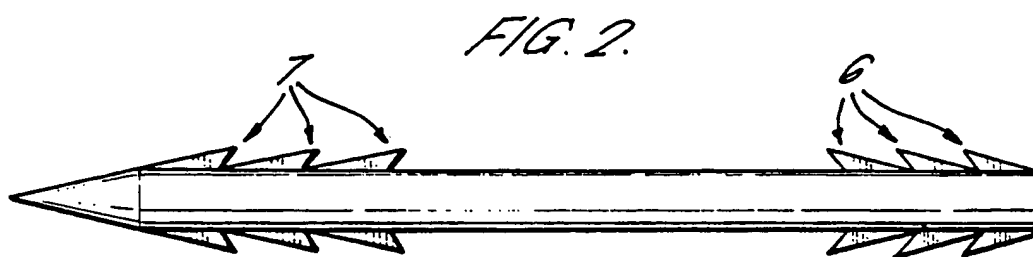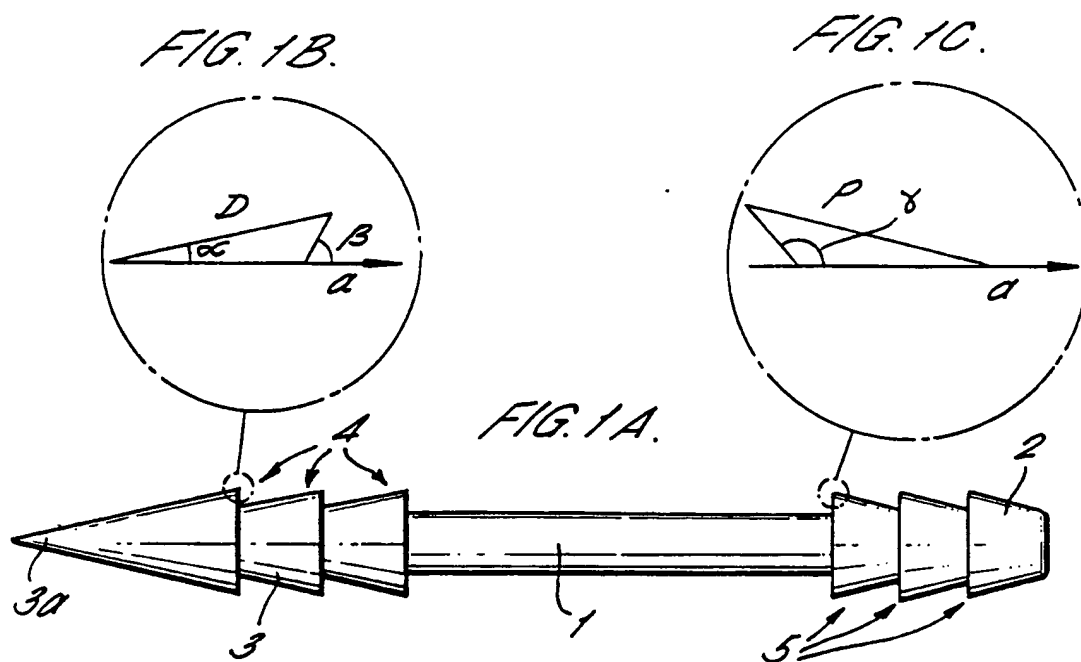

2/6

FIG. 3A.

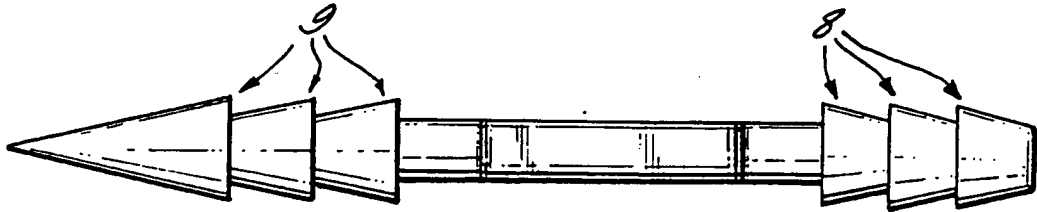


FIG. 3B.


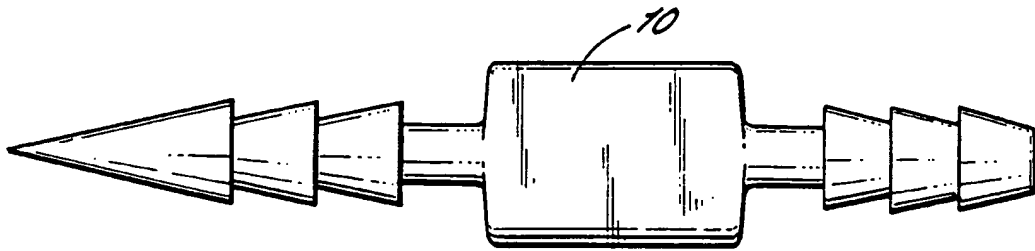


FIG. 3C.



3/6

FIG. 4A.

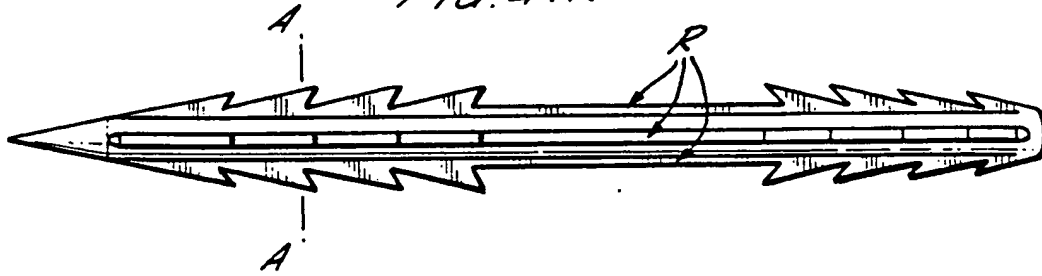


FIG. 4B.




FIG. 5.


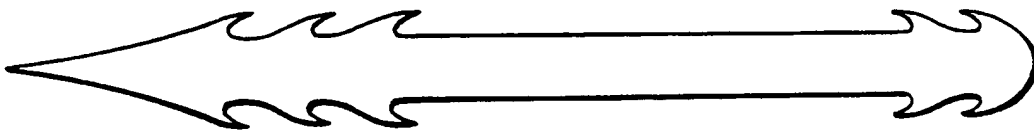


FIG. 6.

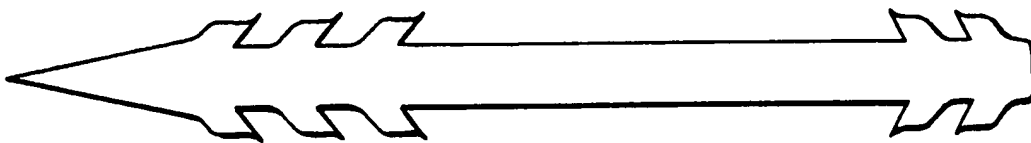

4/6
FIG. 7.

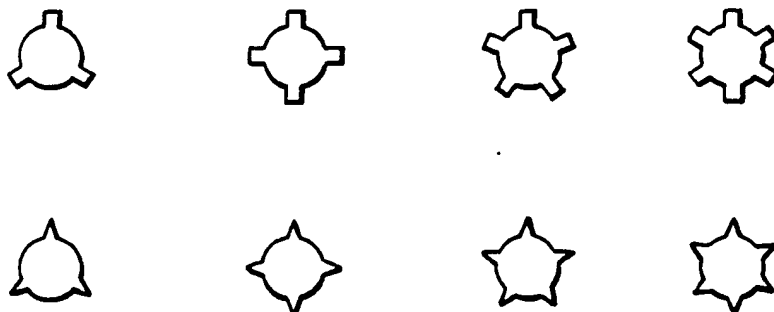


FIG. 8.


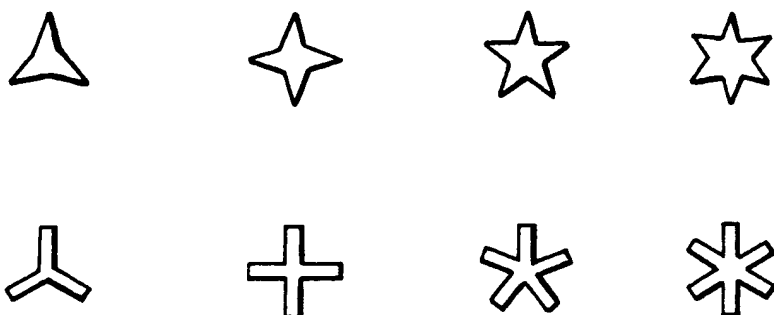






FIG. 9.



FIG. 10.

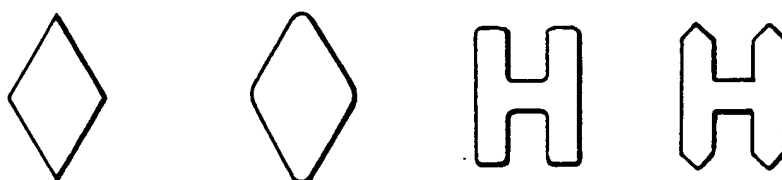

5/6

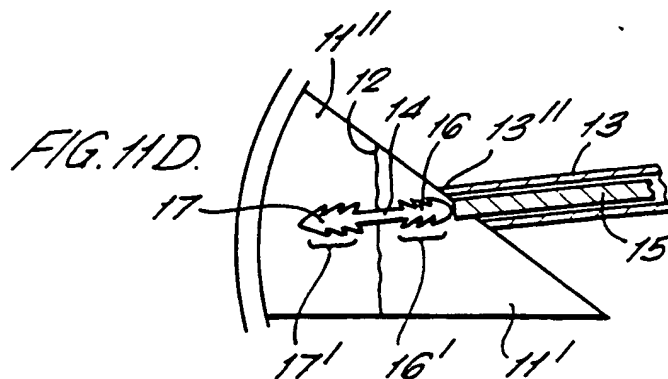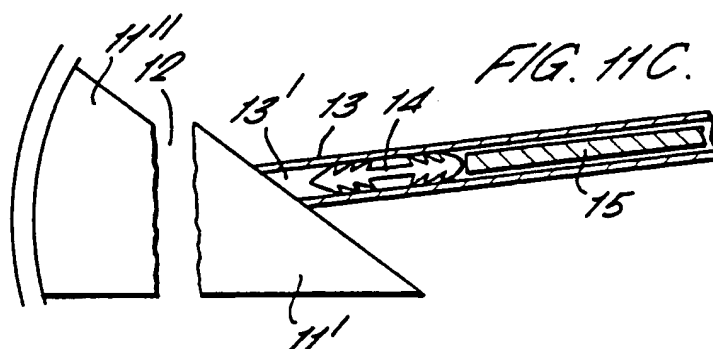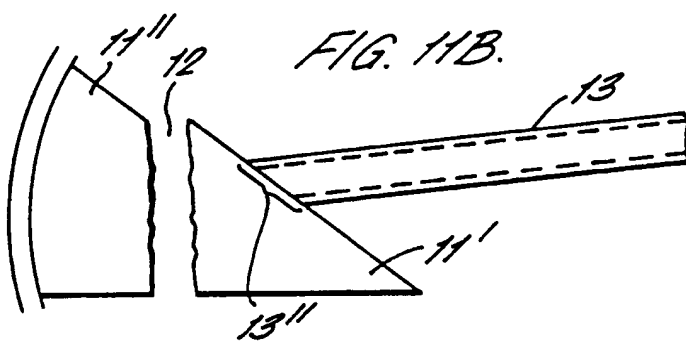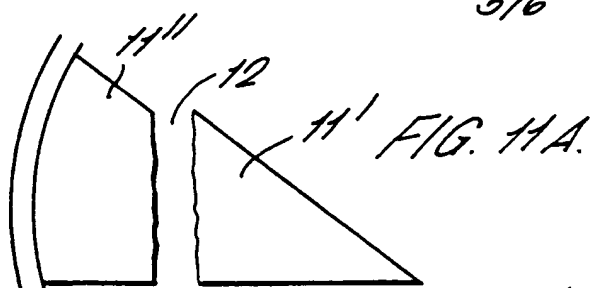

6/6

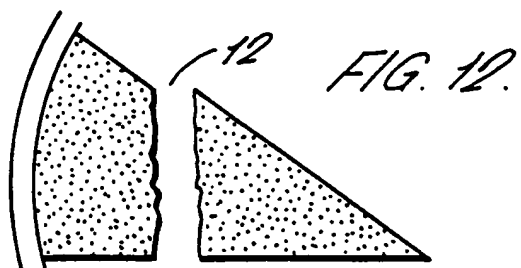


FIG. 13.



FIG. 14.


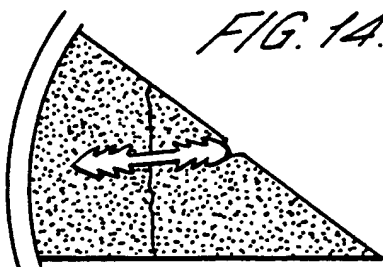


FIG. 15.

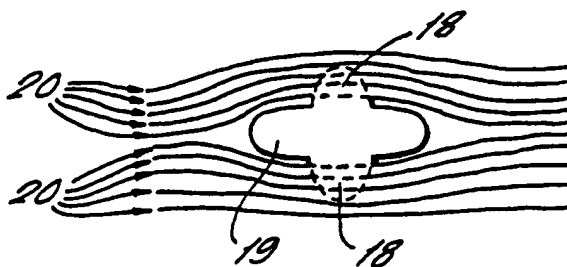

INTERNATIONAL SEARCH REPORT

International Application No

PCT/EP 98/04183

A. CLASSIFICATION OF SUBJECT MATTER
IPC 6 A61B17/064

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
IPC 6 A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 5 643 319 A (GREEN) 1 July 1997 see figures 10,15 ---	1-3
X	US 3 716 058 A (TANNER) 13 February 1973 see figure 3 ---	1,2
X	US 5 398 861 A (GREEN) 21 March 1995 see column 4, paragraph 4; figure 4 ---	1
X	EP 0 770 354 A (USSC) 2 May 1997 see figures 16,19B ---	1
X	EP 0 513 736 A (USSC) 19 November 1992 see figure 1 ---	1
A	US 5 562 704 A (TAMMINMÄKI) 8 October 1996 cited in the application see column 5, line 51 - line 55 --- -/--	5



Further documents are listed in the continuation of box C.



Patent family members are listed in annex.

* Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier document but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- "&" document member of the same patent family

Date of the actual completion of the international search

16 October 1998

Date of mailing of the international search report

23/10/1998

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Barton, S

INTERNATIONAL SEARCH REPORT

International Application No

PCT/EP 98/04183

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 4 873 976 A (SCHREIBER) 17 October 1989 see figures 4,6 ---	4
A	US 5 203 864 A (PHILIPS) 20 April 1993 see figure 1 ---	2
A	WO 97 18762 A (INNOVASIVE) 29 May 1997 -----	

INTERNATIONAL SEARCH REPORT

International application No.

PCT/EP 98/ 04183

Box I Observations where certain claims were found unsearchable (Continuation of item 1 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☒ Claims Nos.: 6
because they relate to subject matter not required to be searched by this Authority, namely:
Rule 39.1(iv) PCT - Method for treatment of the human or animal body by surgery
2. ☐ Claims Nos.:
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box II Observations where unity of invention is lacking (Continuation of item 2 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

☐ The additional search fees were accompanied by the applicant's protest.

☐ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/EP 98/04183

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 5643319 A	01-07-1997	US 5269783 A CA 2100532 A EP 0589306 A CA 2066914 A DE 69201400 T EP 0513736 A US 5374268 A	14-12-1993 22-03-1994 30-03-1994 14-11-1992 13-07-1995 19-11-1992 20-12-1994
US 3716058 A	13-02-1973	NONE	
US 5398861 A	21-03-1995	NONE	
EP 770354 A	02-05-1997	CA 2188114 A	21-04-1997
EP 513736 A	19-11-1992	US 5269783 A CA 2066914 A DE 69201400 T US 5374268 A US 5643319 A	14-12-1993 14-11-1992 13-07-1995 20-12-1994 01-07-1997
US 5562704 A	08-10-1996	FI 920305 A AU 3353793 A CA 2127556 A EP 0623005 A WO 9314705 A JP 7507694 T	25-07-1993 01-09-1993 05-08-1993 09-11-1994 05-08-1993 31-08-1995
US 4873976 A	17-10-1989	AU 4066785 A EP 0174361 A WO 8503857 A	24-09-1985 19-03-1986 12-09-1985
US 5203864 A	20-04-1993	US 5290296 A US 5376097 A US 5290297 A	01-03-1994 27-12-1994 01-03-1994
WO 9718762 A	29-05-1997	AU 1055797 A	11-06-1997